



KONICA MINOLTA

Spectrophotometer

**CM-17d**  
**CM-16d**



Cutting-edge Performance  
and Unmatched Comfort

The Standard in Measuring Color & Light

Giving Shape to Ideas

# Vertical portable spectrophotometer excellent for measuring small samples and curved surfaces


The CM-17d has a camera viewfinder for easy positioning.

The CM-16d is designed for simplicity and offers excellent cost performance.



Spectrophotometer

**CM-17d | CM-16d**

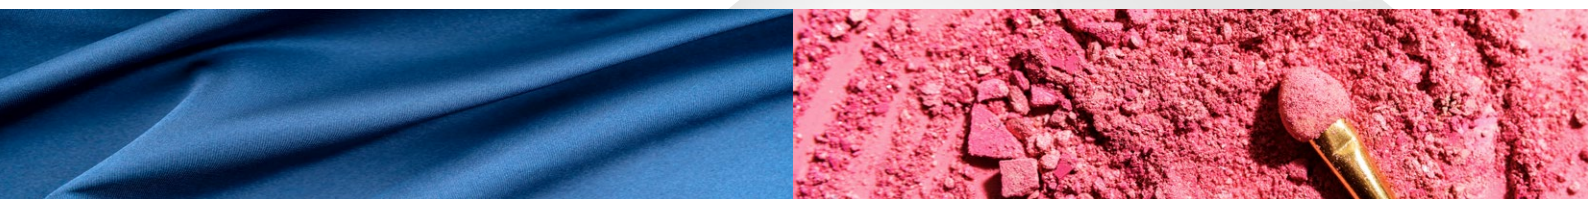

## ■ Simple to Configure and Ease of Use

Ergonomically designed to be easy to grip. It can be used in a wide range of measurement scenarios, including one-handed work, vertical orientation, and measurement of small objects and curved surfaces. Stress-free hardware design includes easy positioning with the camera viewfinder\*<sup>1</sup>, improved visibility with a slight tilt of the operation screen, and a comfortable workspace with wireless connectivity\*<sup>2</sup>.


\*1 Camera viewfinder is a feature of CM-17d only.

\*2 WLAN/Bluetooth module (option) is required.




## ■ Higher accuracy and shorter measurement time

The CM-17d has adopted a  $d_i:8^\circ$  and  $d_e:8^\circ$  integrating sphere compatible with the previous CM-700d series. Along with the improved measurement accuracy of black color, the CM-17d also improves efficiency with shorter measurement times.

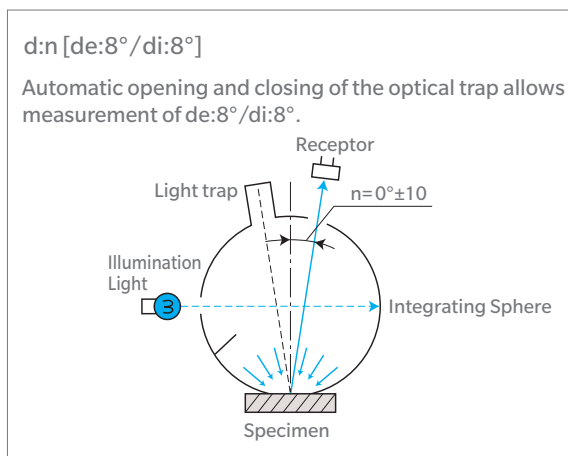

### Measurement time comparison for five consecutive measurements

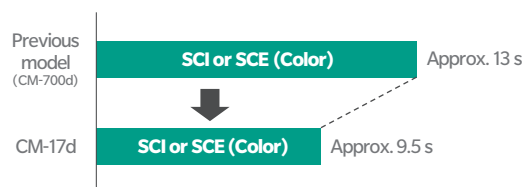

\* Time per measurement: CM-700d 1s, CM-17d 0.7s  
Minimum measurement interval: CM-700d 2s, CM-17d 1.5s

## ■ Various measurement examples utilizing optional accessories

The vertical leveling jig is useful when the main unit is turned upside down for measurement. The tripod hole on the front of the body can also be used to hold the instrument in place.




Vertical Leveling Jig



\*Product image for illustration purposes only.

## ■ Color Data Software SpectraMagic NX2 (Option)

SpectraMagic NX2 is color management software that gives users a customizable screen display and a wide range of functions for operating and transferring data between their Spectrophotometer or Chroma Meter to their computer for further analysis. Users can display data lists and create color difference graphs and spectral graphs to assist in color management that requires judgment based on numerous values and indicators.

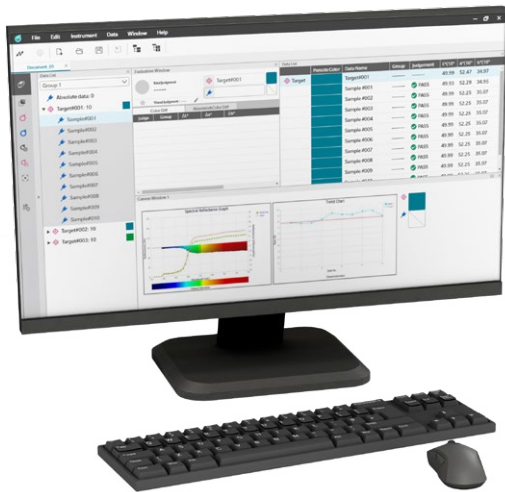

Wireless connection\*



\* WLAN/Bluetooth module (Option) is required for wireless connection.  
A wired connection via cable is also possible.

You can see the details in the catalog from the following 2D code. ↓  
[SpectraMagic NX2 website](#)





## ■ Wavelength Analysis & Adjustment for high stability

WAA (Wavelength Analysis & Adjustment) provides worry-free, higher-reliability measurements and minimizes system problems by suppressing shifts in measurement. WAA is available free of charge for the first year after purchase of the CM-17d series. After the second year, WAA can be continued as an add-on to the inspection and calibration service.

## ■ Cradle for charging and zero calibration

When not in use, the instrument can be placed on the Cradle\* to charge the battery, and provide a safe stowage. Also serves as a zero calibration table, allowing calibration work to be performed while the unit is in place.

\* Standard accessories only for CM-17d



White Calibration Cap

Cradle for charging  
And Zero Calibration



## Try CM-17d with Augmented Reality.

Scan the 2D code to see product size and design on your iPhone.

- \* You can only use it with an iPhone.
- \* Please refer to the specification for the dimensions of the product.
- \* All the content copyrights belong to Konica Minolta, Inc.




# CM-17d Series spectrophotometers can be used in a wide range of industries.

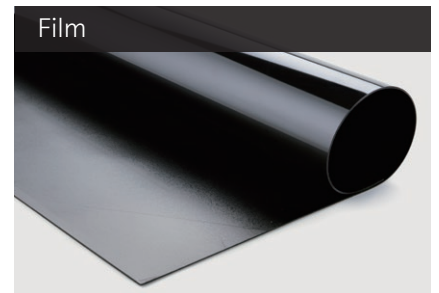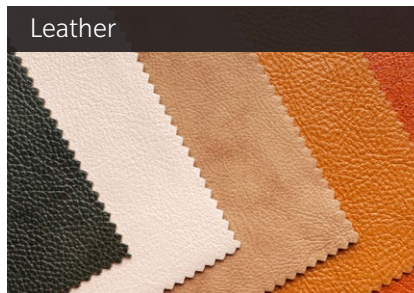


## ■ Spectrophotometer Configuration Tool CM-CT1 Ver. 1.5 or later

The CM-CT1 gives manufacturers the means for easily and quickly setting up their spectrophotometers. Moreover, when multiple devices are used or when the same conditions need to be set amongst multiple factories or suppliers, settings can be compiled into a file and shared.

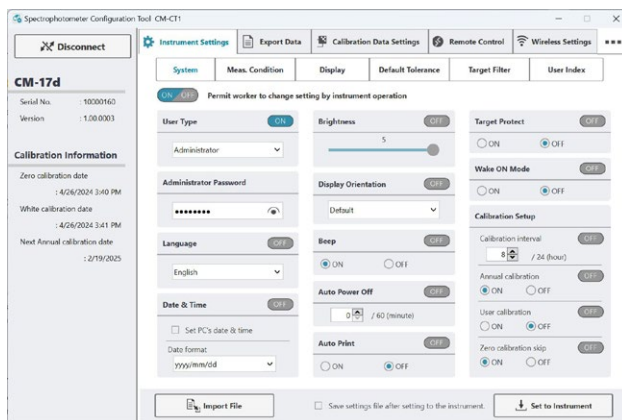

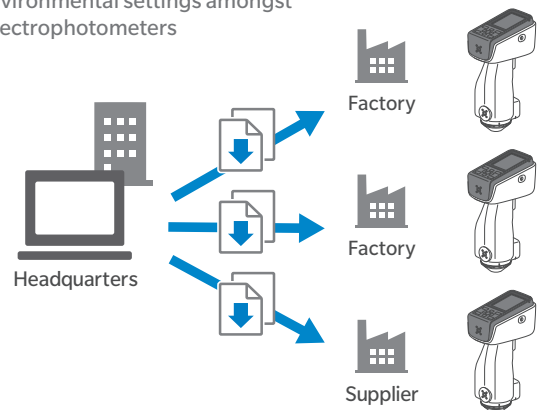


Easily unify measurement conditions and environmental settings amongst spectrophotometers




## Spectrophotometer Configuration Tool CM-CT1


- OS : Windows® 10 Pro 64 bit Version 1903 or higher / Windows® 11 Pro
  - CPU : 2.0 GHz equivalent or faster
  - Memory : 2 GB or more
  - Hard disk : 10 GB or more of free space for installation
  - Other : USB port (For connecting to spectrophotometers and SpectraMagic NX2 dongle)
- Windows® is a trademark or registered trademark of Microsoft Corporation in the USA and other countries.

## System Diagram


-  Standard Accessories
-  Optional Accessories
-  Connection possible

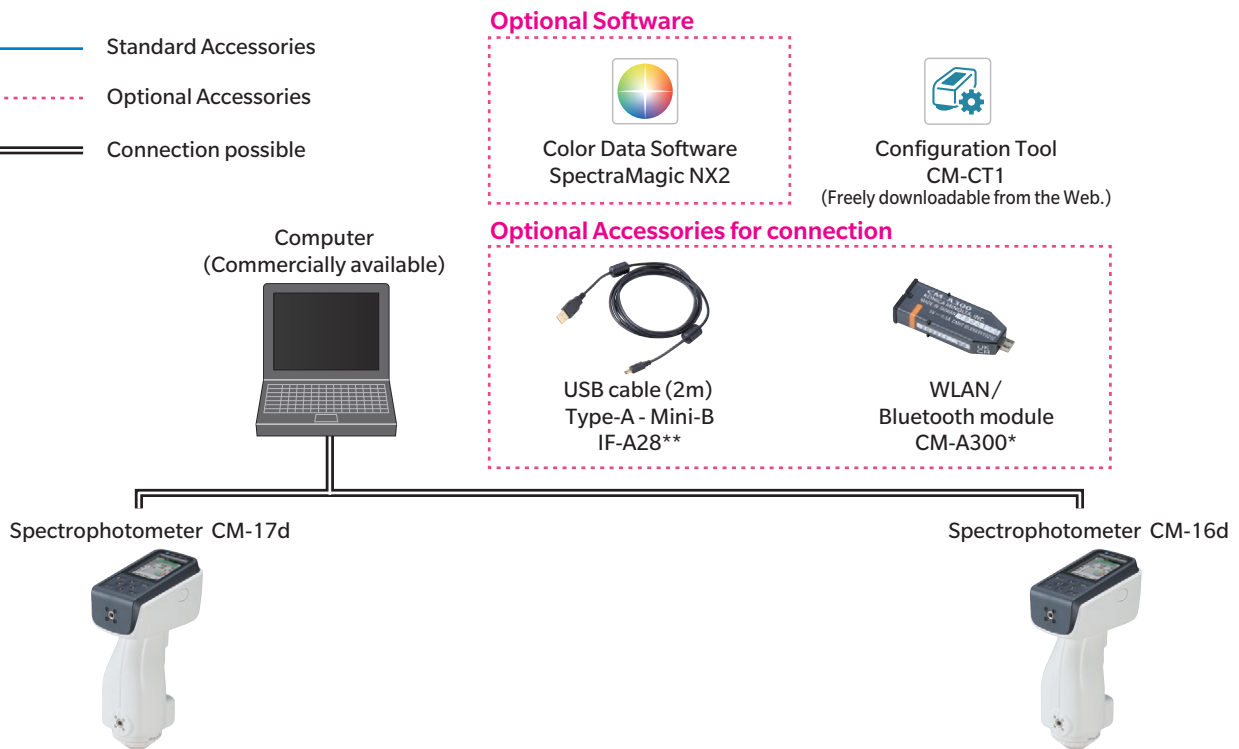

### Standard Accessories for CM-17d

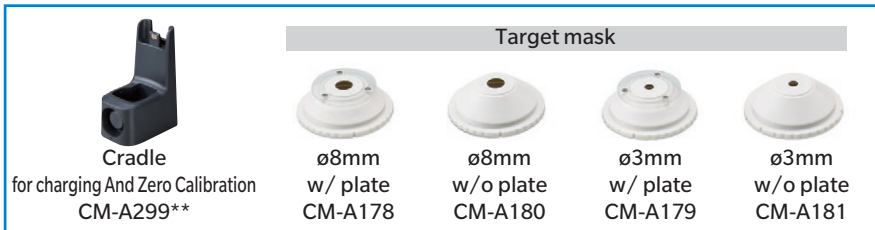

### Standard Accessories for CM-16d

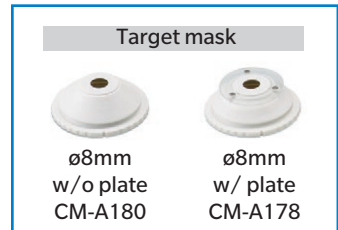

### Standard Accessories



### Optional Accessories




\* Depending on the location, some accessories may not be available.

\*\* May be included as a standard accessory in some regions.

# Specifications

	CM-17d	CM-16d
Illumination/viewing system	di:8°, de:8° (diffuse illumination: 8° viewing), SCI (specular component included) / SCE (specular component excluded) switchable	
Applicable standards for illumination/viewing system	Conforms to ISO7724/1, CIE No.15 (2004), ASTM E 1164 (SCI), DIN5033 Teil7, JIS Z 8722 Condition c standard	
Integrating sphere	Ø40 mm	
Detector	Dual 32-element silicon photodiode arrays	
Spectral separation device	Planar diffraction grating	
Wavelength range	400 nm to 700 nm	
Measurement wavelength pitch	10 nm	
Half bandwidth	Approx. 10 nm	
Reflectance range	0 to 175%; Resolution: 0.01%	
Light source	Pulsed xenon lamp (with UV cut filter)	
Measurement time	Approx. 0.7 s (Measurement mode: SCI or SCE, from pressing trigger button to measurement completion)	
Minimum measurement interval	Approx. 1.5 s (Measurement mode: SCI or SCE)	
Battery performance	Approx. 2,000 measurements (approx. 1,000 measurements when using Optional WLAN/Bluetooth module) when measurements are taken at 10-second intervals at 23°C with the dedicated lithium battery, without using camera viewfinder	
Measurement area/illumination area	MAV:Ø8 mm/Ø11 mm SAV:Ø3 mm/Ø6 mm *Can be changed by replacing the target mask and switching the lens position	MAV:Ø8 mm/Ø11 mm
Repeatability	Standard deviation within ΔE*ab 0.02 (When a white calibration plate is measured 30 times at 5-second intervals after white calibration under Konica Minolta standard conditions)	Standard deviation within ΔE*ab 0.04 (When a white calibration plate is measured 30 times at 5-second intervals after white calibration under Konica Minolta standard conditions)
Inter-instrument agreement	Within ΔE*ab 0.12 (Based on average for 12 BCRA Series II color tiles; MAV SCI; compared to values measured with a master body under Konica Minolta standard conditions)	Within ΔE*ab 0.2 (Based on average for 12 BCRA Series II color tiles; MAV SCI; compared to values measured with a master body under Konica Minolta standard conditions)
Display	2.7-inch TFT color LCD with reversible portrait viewing mode	
Internal performance check <sup>1</sup>	WAA (Wavelength Analysis & Adjustment) Technology	
Interface	USB 2.0; WLAN (IEEE 802.11 b/g/n)/Bluetooth(Ver.4.1, SPP-compatible.) Optional WLAN/Bluetooth module required <sup>2,3</sup>	
Camera viewfinder function	Using internal camera; Images can be shown on display	—
Observer	2° Standard Observer, 10° Standard Observer	
Illuminant	A,C,D50,D65,F2,F6,F7,F8,F10,F11,F12,ID50,ID65,LED-B1,LED-B2,LED-B3,LED-B4,LED-B5,LED-BH1,LED-RGB1,LED-V1,LED-V2,User-defined illuminant <sup>4</sup> (Max. 3 types) (Simultaneous evaluation with two light sources possible)	
Display items	Colorimetric values/graph, color difference values/graph, spectral graph, pass/fail judgment, pseudocolor	
Color spaces	L*a*b*, L*C*h, Hunter Lab, Yxy, XYZ, and color difference in these spaces; Munsell (C)	
Indices	MI, WI (ASTM E313-73/ASTM E313-98);YI (ASTM E313-73, ASTM D1925);ISO brightness (ISO2470);WI/Tint (CIE);Tristimulus Strength;Opacity; Grey scale (ISO 105-A05);gloss value; User index <sup>5</sup> , Blackness (My) (ISO18314-3/DIN55979);Jetness (Mc) (ISO18314-3);Undertone (dM) (ISO18314-3)	
Color difference equations	ΔE*ab (CIE1976); ΔE*94 (CIE1994); ΔE00 (CIEDE2000); CMC (l:c); Hunter ΔE; DIN99a; FMC-2; ΔE*94 (Special) <sup>6</sup>	
Data memory	1,000 target data + 5,000 sample data	
Power	AC power supply	USB Type-C AC adapter (Power Delivery compatible, 15 W or more)
	Battery	Lithium-ion battery (removable)
	USB charging	USB bus power (with lithium-ion battery installed)
Charging time	Approx. 3.5 h (rapid charge) / Approx. 6 h (standard)	
Size	Approx. 79(W)×230(H)×128(D) mm	
Weight	Approx.700 g (Lithium-ion battery included)	Approx.660 g (Lithium-ion battery included)
Operating temperature/humidity range	Temperature: 5 to 40°C; Relative humidity: 80% or less (at 35°C) with no condensation	
Storage temperature/humidity range	Temperature: 0 to 45°C; Relative humidity: 80% or less (at 35°C) with no condensation	

## Dimensions (Units: mm)

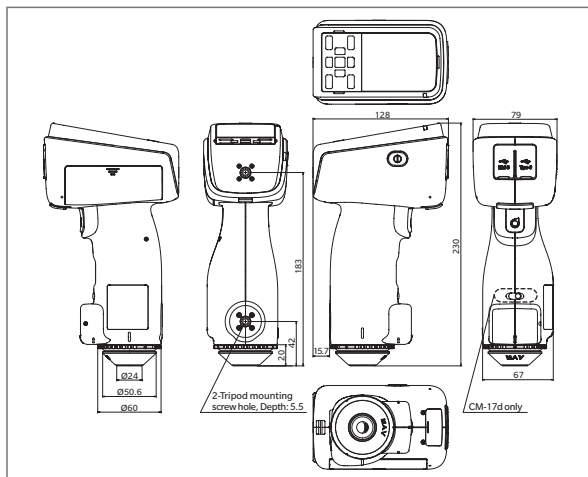

- \*1 The WAA function enables wavelength diagnosis and wavelength correction of the instrument. This function is available free of charge for the first year after purchase, and can be continued after the second year by having the instrument serviced and calibrated.
- \*2 Requires optional accessory WLAN / Bluetooth module (CM-A300).
- \*3 WLAN security supports WPA2-PSK (WPA2-Personal) and WPA-PSK (WPA-Personal) for the AdHoc method, and WPA3-PSK (WPA3-Personal), WPA2-PSK (WPA2-Personal) and WPA-PSK (WPA-Personal) for the Infrastructure method.
- \*4 Optional Color Data Software SpectraMagic NX2 Pro (Ver. 1.3 or later) is required for setting user-configured illuminants.
- \*5 Spectrophotometer Configuration Tool CM-CT1 Ver. 1.5 or later and a valid Color Data Software SpectraMagic NX2 license are required for setting user indices.
- \*6 When comparing two colors, please use ΔE\*94(Special) if one of them is not specified as the standard.

- KONICAMINOLTA, the Konica Minolta logo and symbol mark, "Giving Shape to Ideas" and SpectraMagic are registered trademarks or trademarks of Konica Minolta, Inc.
- Bluetooth® is a registered trademark of Bluetooth SIG, Inc. and is used under license agreement.
- iPhone® is a registered trademark of Apple Inc., registered in the U.S. and other countries.
- Displays shown are for illustration purpose only.
- The specifications and appearance shown herein are subject to change without notice.

**SAFETY PRECAUTIONS**

For correct use and for your safety, be sure to read the instruction manual before using the instrument.

- Always connect the instrument to the specified power supply voltage.

Improper connection may cause a fire or electric shock.

ISO Certifications of KONICA MINOLTA, Inc., Sakai Site



JQA-QMA15888  
Design, development, manufacture/  
manufacturing management, calibration, and  
service of measuring instruments



JQA-E-80027  
Design, development,  
manufacture, service and sales  
of measuring instruments

<b>KONICA MINOLTA, INC.</b>	Osaka, Japan			
<b>Konica Minolta Sensing Americas, Inc.</b>	New Jersey, U.S.A.	PHONE: (888)473-2656 (in USA), +1(201)236-4300 (outside USA)	FAX: +1(201)785-2480	E-Mail: service.us@konicaminolta.com
<b>Konica Minolta Sensing Europe B.V.</b>	European HQ / BENELUX German Office French Office UK Office Italian Office Swiss Office Nordic Office Polish Office	Nieuwegein, Netherlands München, Germany Roissy CDG Cedex, France Warrington, United Kingdom Cinisello Balsamo, Italy Dietikon, Switzerland VÄSTRA FRÖLUNDA, Sweden Wrocław, Poland	PHONE: +31(0)30 248-1193 PHONE: +49(0)89 4357 156 0 PHONE: +33(0)1 80 11 10 70 PHONE: +44(0)1925 467300 PHONE: +39 02849488.00 PHONE: +41(0)43 322-9800 PHONE: +46(0)31 7099464 PHONE: +48(0)71 73452-11	E-Mail: info.benelux@seu.konicaminolta.eu E-Mail: info.germany@seu.konicaminolta.eu E-Mail: info.france@seu.konicaminolta.eu E-Mail: info.uk@seu.konicaminolta.eu E-Mail: info.italy@seu.konicaminolta.eu E-Mail: info.switzerland@seu.konicaminolta.eu E-Mail: info.nordic@seu.konicaminolta.eu E-Mail: info.poland@seu.konicaminolta.eu
<b>Konica Minolta (CHINA) Investment Ltd.</b>	SE Sales Division Beijing Office Guangzhou Office Chongqing Office Qingdao Office Wuhan Office Shenzhen Office Xiamen Office	Shanghai, China Beijing, China Guangzhou, China Chongqing, China Shandong, China Hubei, China Shenzhen, China Xiamen, China	PHONE: +86(0)21-6057-1089 PHONE: +86(0)10-8522 1551 PHONE: +86(0)20-3826 4220 PHONE: +86(0)23-6773 4988 PHONE: +86(0)532-8079 1871 PHONE: +86(0)27-6885 0586 PHONE: +86(0)755-2868 7535 PHONE: +86(0)592-7107 399	E-Mail: hcn_sensing@gcp.konicaminolta.com E-Mail: hcn_sensing@gcp.konicaminolta.com E-Mail: hcn_sensing@gcp.konicaminolta.com E-Mail: hcn_sensing@gcp.konicaminolta.com E-Mail: hcn_sensing@gcp.konicaminolta.com E-Mail: hcn_sensing@gcp.konicaminolta.com E-Mail: hcn_sensing@gcp.konicaminolta.com E-Mail: hcn_sensing@gcp.konicaminolta.com
<b>Konica Minolta Sensing Singapore Pte. Ltd.</b>	Singapore	PHONE: +65 6563-5533		E-Mail: se-service.sg@konicaminolta.com
<b>Konica Minolta Sensing Korea Co., Ltd.</b>	Korean HQ Cheonan Office	Goyang-si, Korea Cheonan-si, Korea	PHONE: +82(0)2-523-9726 PHONE: +82(0)41-556-9726	E-Mail: se.korea@konicaminolta.com E-Mail: se.korea@konicaminolta.com

Addresses and telephone/fax numbers and e-mail address are subject to change without notice.  
For the latest contact information, please refer to KONICA MINOLTA Worldwide Offices web page:

<https://konicaminolta.com/instruments/network>